



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Zauberland Alpakas/Hartwig Kraft-Von Wedel
Wiederodaer Str. 2
Remsa 04769 Germany

06/26/15

Test No: 905003


Animal and Sample Description

Animal Name: AIG Ditte (AIG Mr. Hagert)
Breed: Alpaca(Huacaya)
Sex: Female
Color: Lt Silver Grey

Animal ID: 94500001293963
Sample Location: Mid Side
Sample Date: 05/25/15
Age: 08/21/14

Laboratory Data

Mean Fiber Diameter: 17.5 microns
Standard Deviation: 3.7 microns
Coefficient of Variation: 20.8 %
Fibers Greater Than 30 microns: 0.6 %

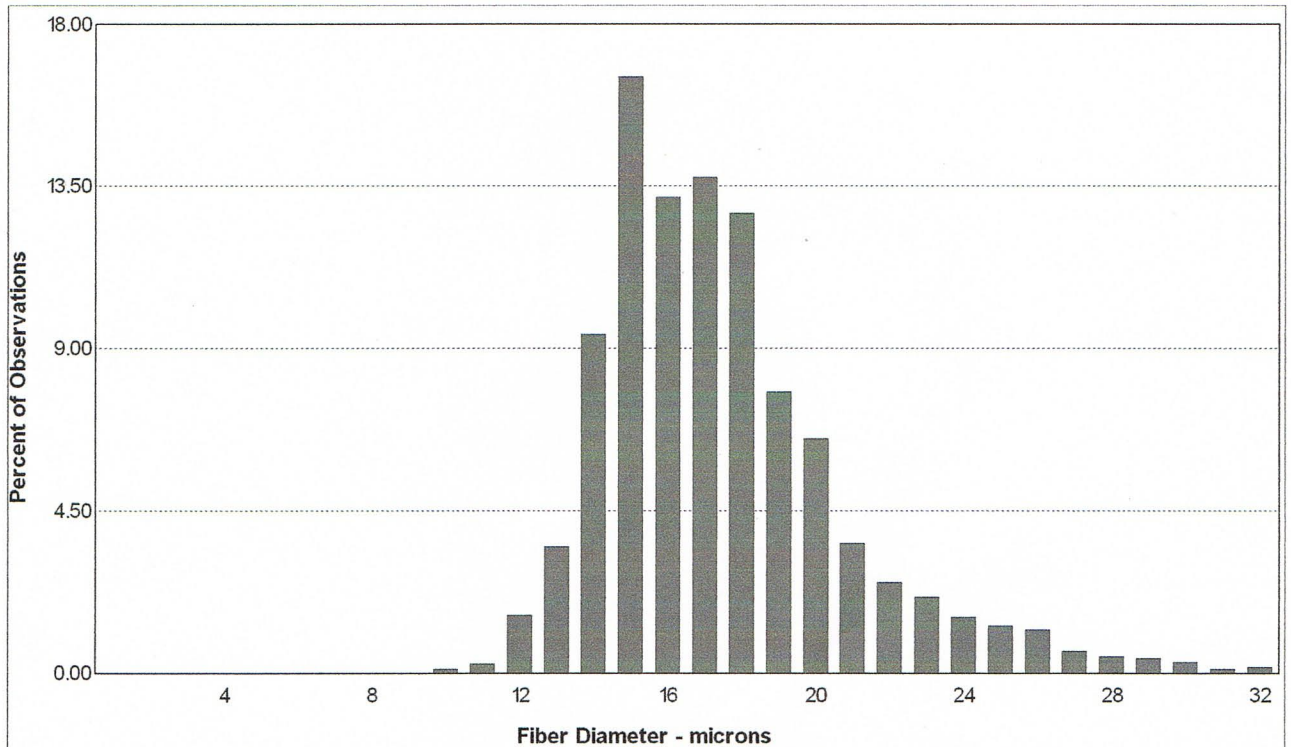

This Test Performed According to I.W.T.O Method 12